Neutron Spectra Measured with Time-of-Flight Detectors on the National Ignition Facility

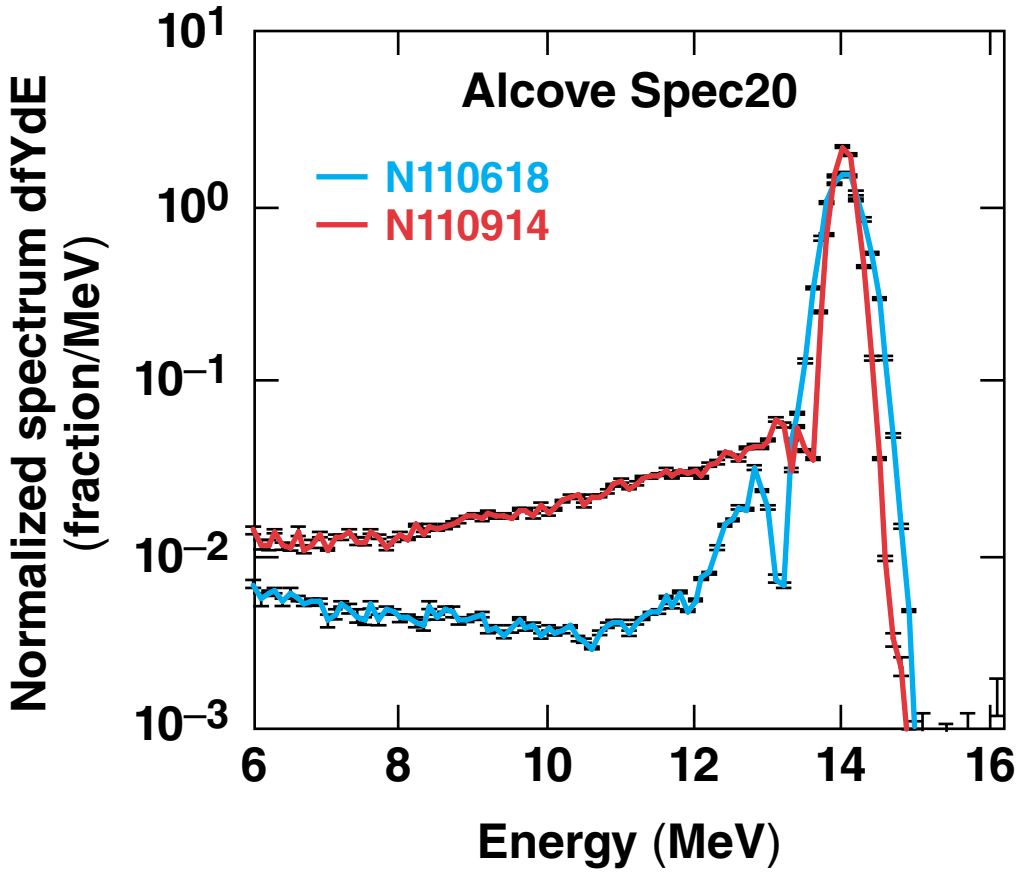

J. P. Knauer
University of Rochester
Laboratory for Laser Energetics

53rd Annual Meeting of the
American Physical Society
Division of Plasma Physics
Salt Lake City, UT
14–18 November 2011

Summary

High-quality data from NIF Spec20 detectors make it possible for neutron spectra to be calculated from a deconvolution

- Instrument response function (IRF) determined from *in-situ* measurements
- Spec20 detectors probe NIF implosions from two different lines-of-sight
- Neutron spectra are calculated with an error analysis built into the deconvolution

NIF nTOF development has been done by a large team of collaborators

Y. Yu. Glebov, D. D. Meyerhofer, T. C. Sangster, and C. Stoeckl

University of Rochester
Laboratory for Laser Energetics

E. J. Bond, J. A. Caggiano, T. J. Clancy, M. J. Eckart, S. Friedrich, R. Hatarik, R. A. Lerche, A. J. Mackinnon, J. McNaney, M. J. Moran, and D. H. Munro

Lawrence Livermore National Laboratory

S. J. Padalino

State University of New York, Geneseo
Department of Physics and Astronomy

J. D. Kilkenny

General Atomics, Inc.

Several nTOF detectors are distributed around the NIF target chamber

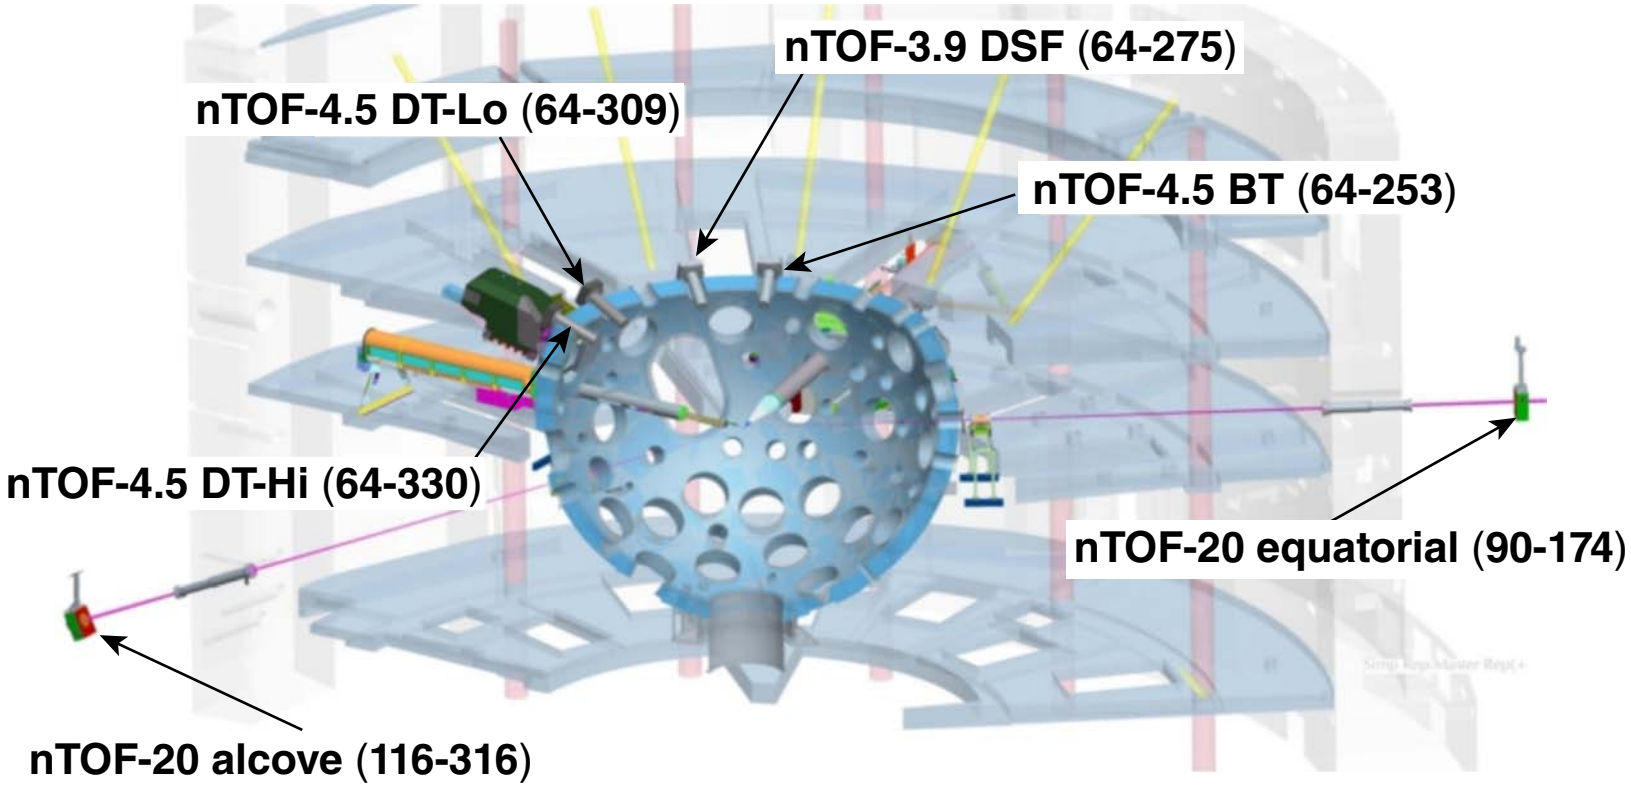

Neutron down scatter is measured along four lines-of-sight.

E20356

DSR measurements sample ρR of large-opening angle cones about the diagnostic direction

Neutrons scattered from tritium and deuterium

Instrument – (θ, ϕ)
3.9 m DSF – (64, 275)
MRS – (77, 324)
Alcove Spec20 – (116, 316)
Equator Spec20 – (90, 174)

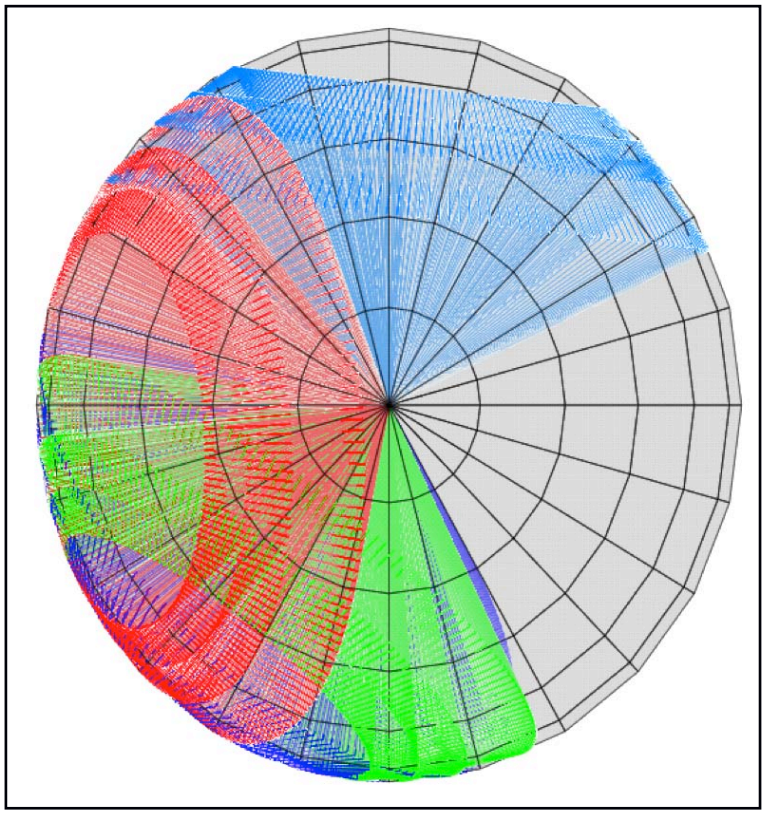

The average of all DSR measurements represents the average target ρR.

E20357

Instrument response functions (IRF's) are constructed with a dynamic range of 10^3

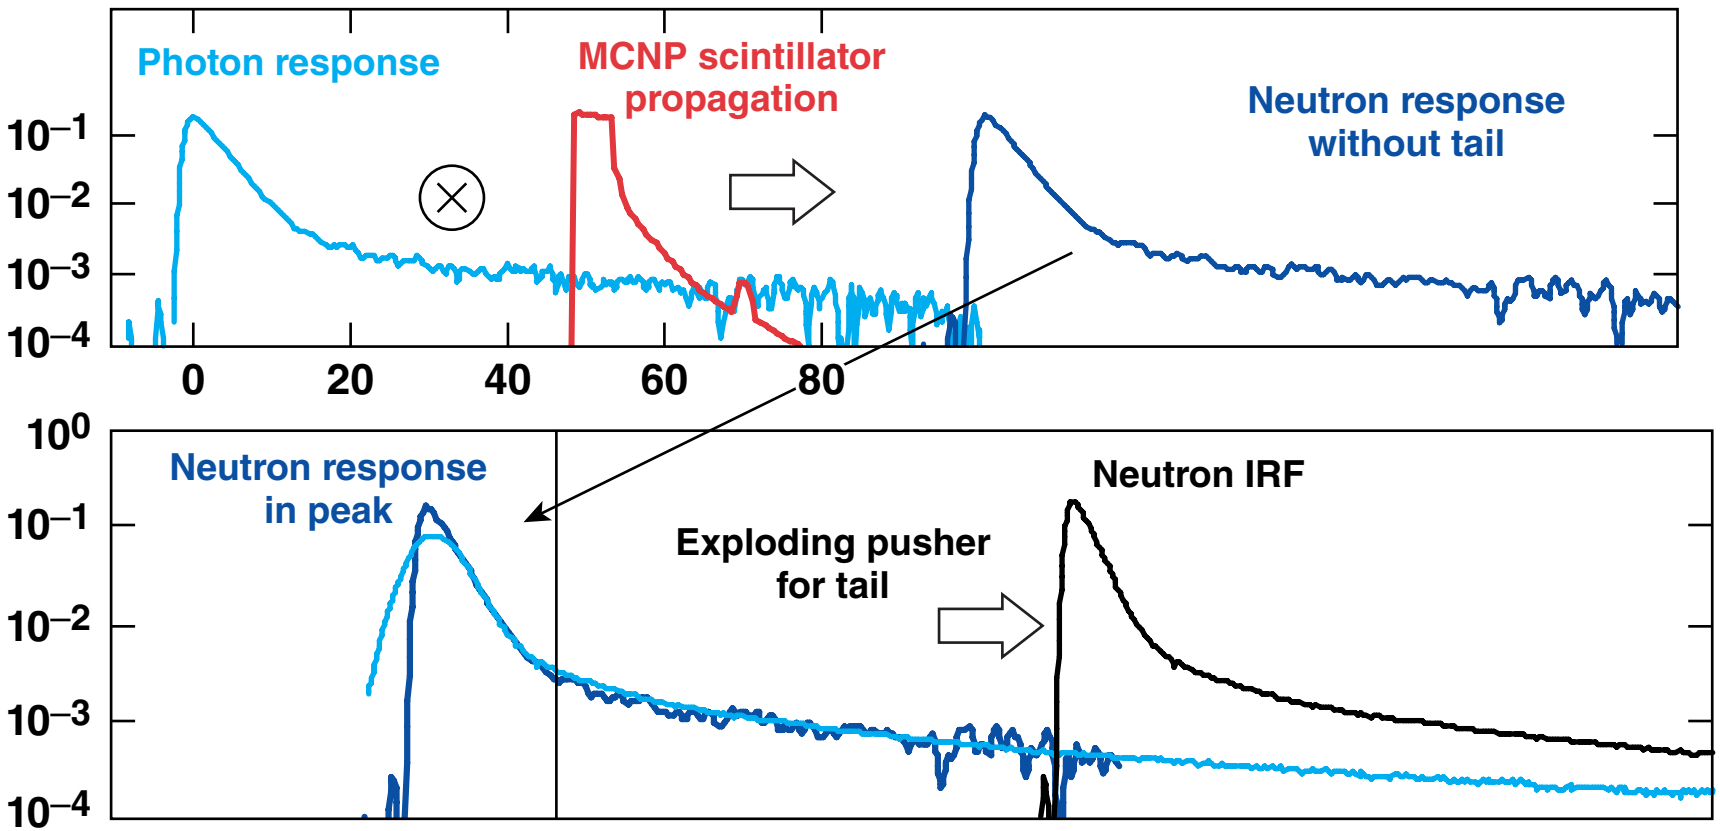

Instrument IRF is calculated from x-ray data, neutron propagation in scintillator calculated from MCNP, and exploding-pusher data.

E20358

Spec20 deconvolution uses a Wiener-filtered FFT technique

- Use signal-to-noise to determine number of points for FFT analysis (typically 4096)
- Use same number of points in data for leading and trailing noise windows
- FFT data, noise, and IRF
- Construct Wiener filter from power spectrum from IRF and noise using a Lagrangian multiplier
- Calculate deconvolved signal from inverse FFT of (WF*[FFT(data)/FFT(IRF)]
- Optimize Lagrangian multiplier by minimizing under- and overshoots in signal (subjective)
- Convert data to energy domain
- Calculate scalars DSF, T_{ion}, yield
- Calculate energy spectrum with 50-keV resolution

E20359

Errors propagated throughout deconvolution analysis

- δ FFT from noise
- δ signal from δ FFT
- δ spectrum from δ signal
- σ scalars

Exploding-pusher neutron spectra agree but may show a difference between 1.5- and 2.1-mm shells

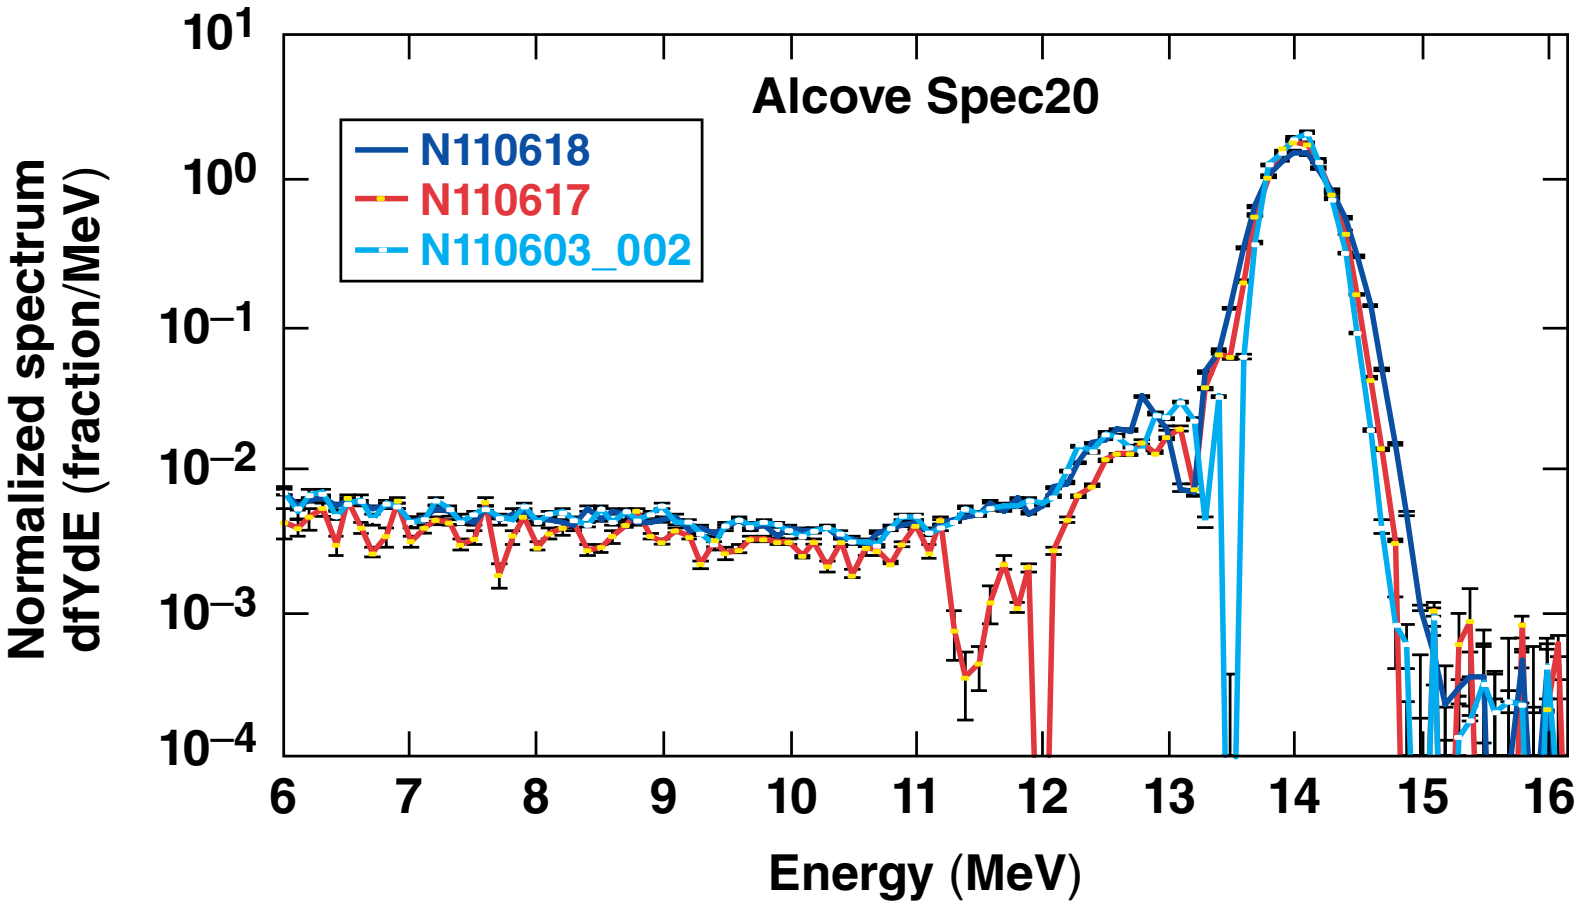

E20361

Convolution of DT peak with IRF shows scattered neutrons

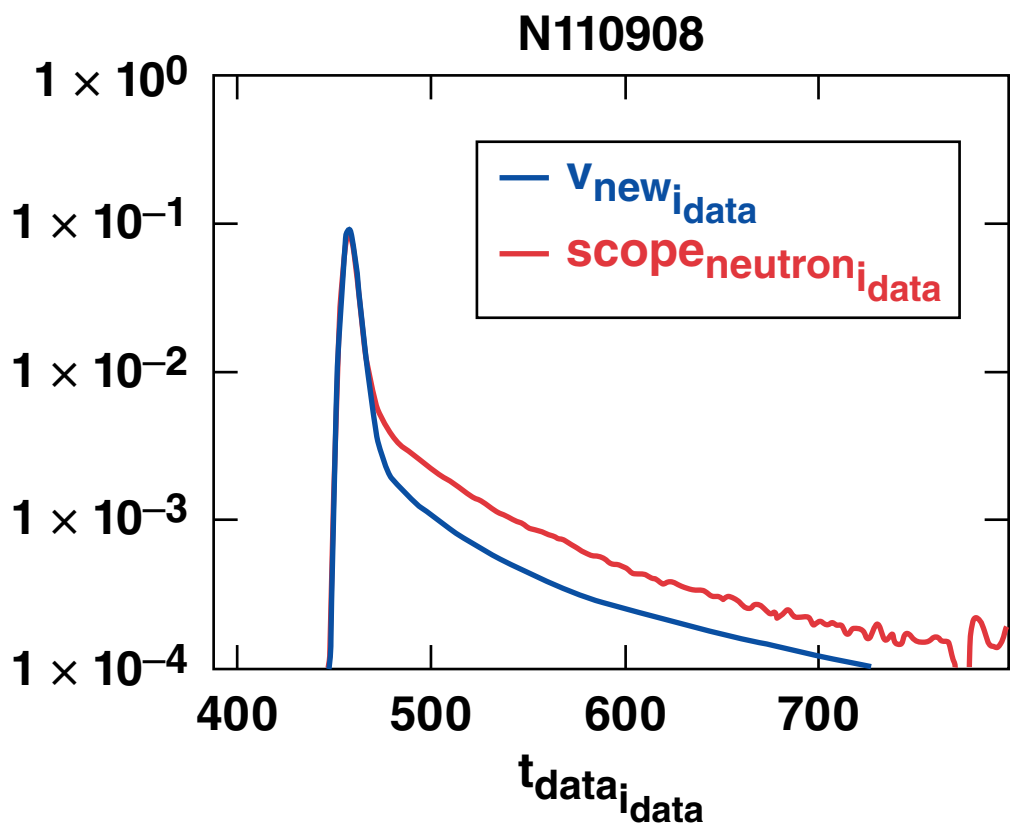

E20362

Down-scattered neutrons are clearly seen in deconvolved spectra

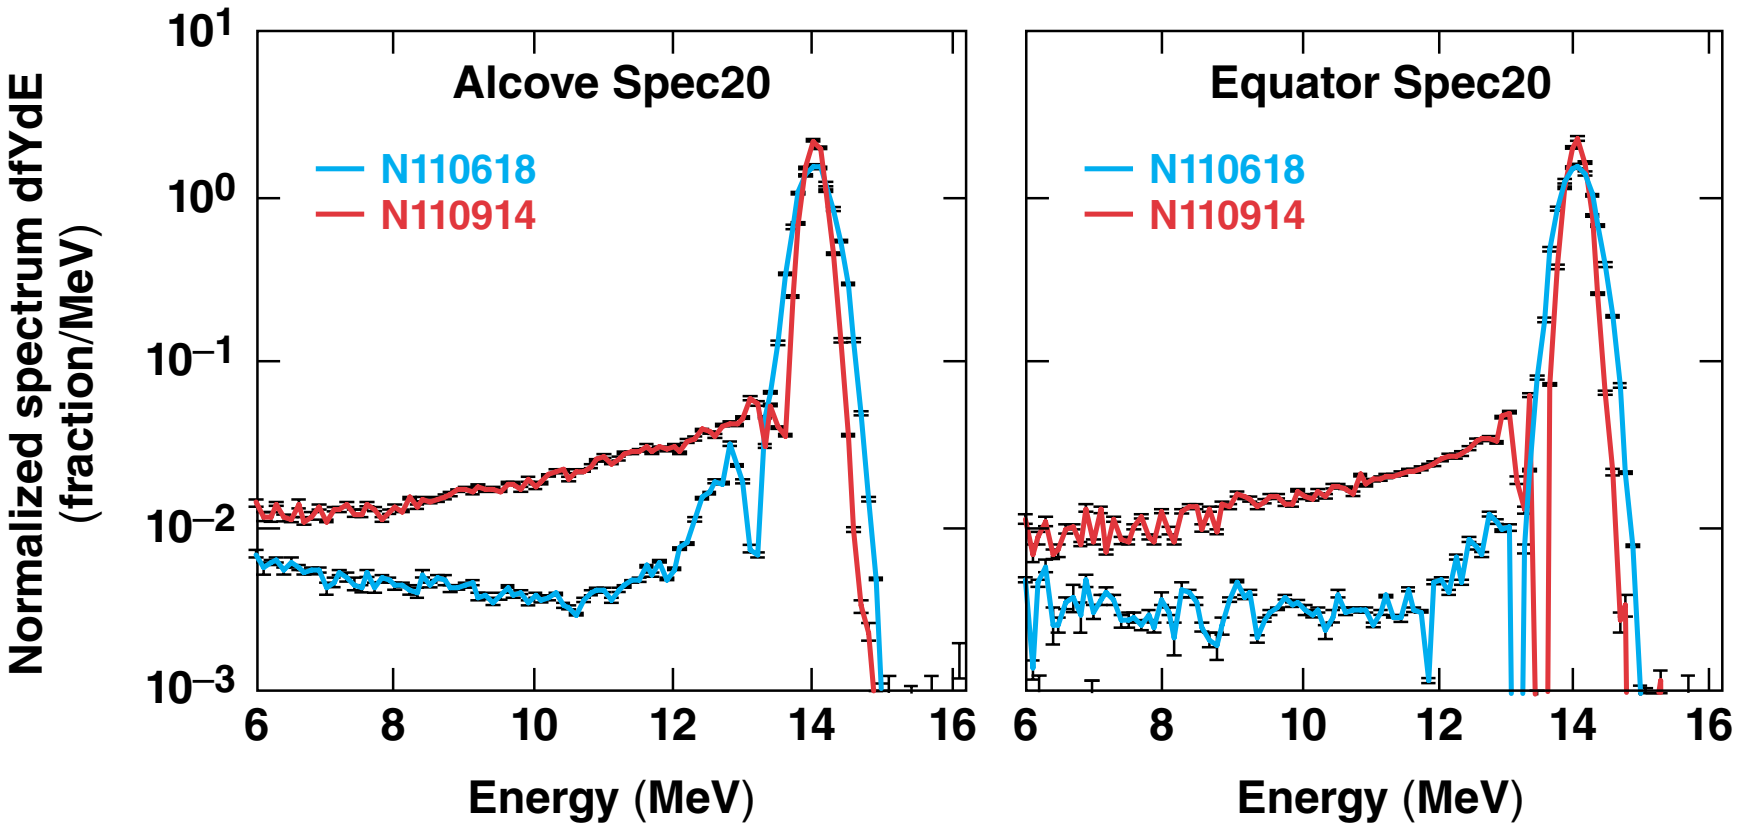

E20363

THD spectra show the TT neutrons in both alcove and equator Spec20's

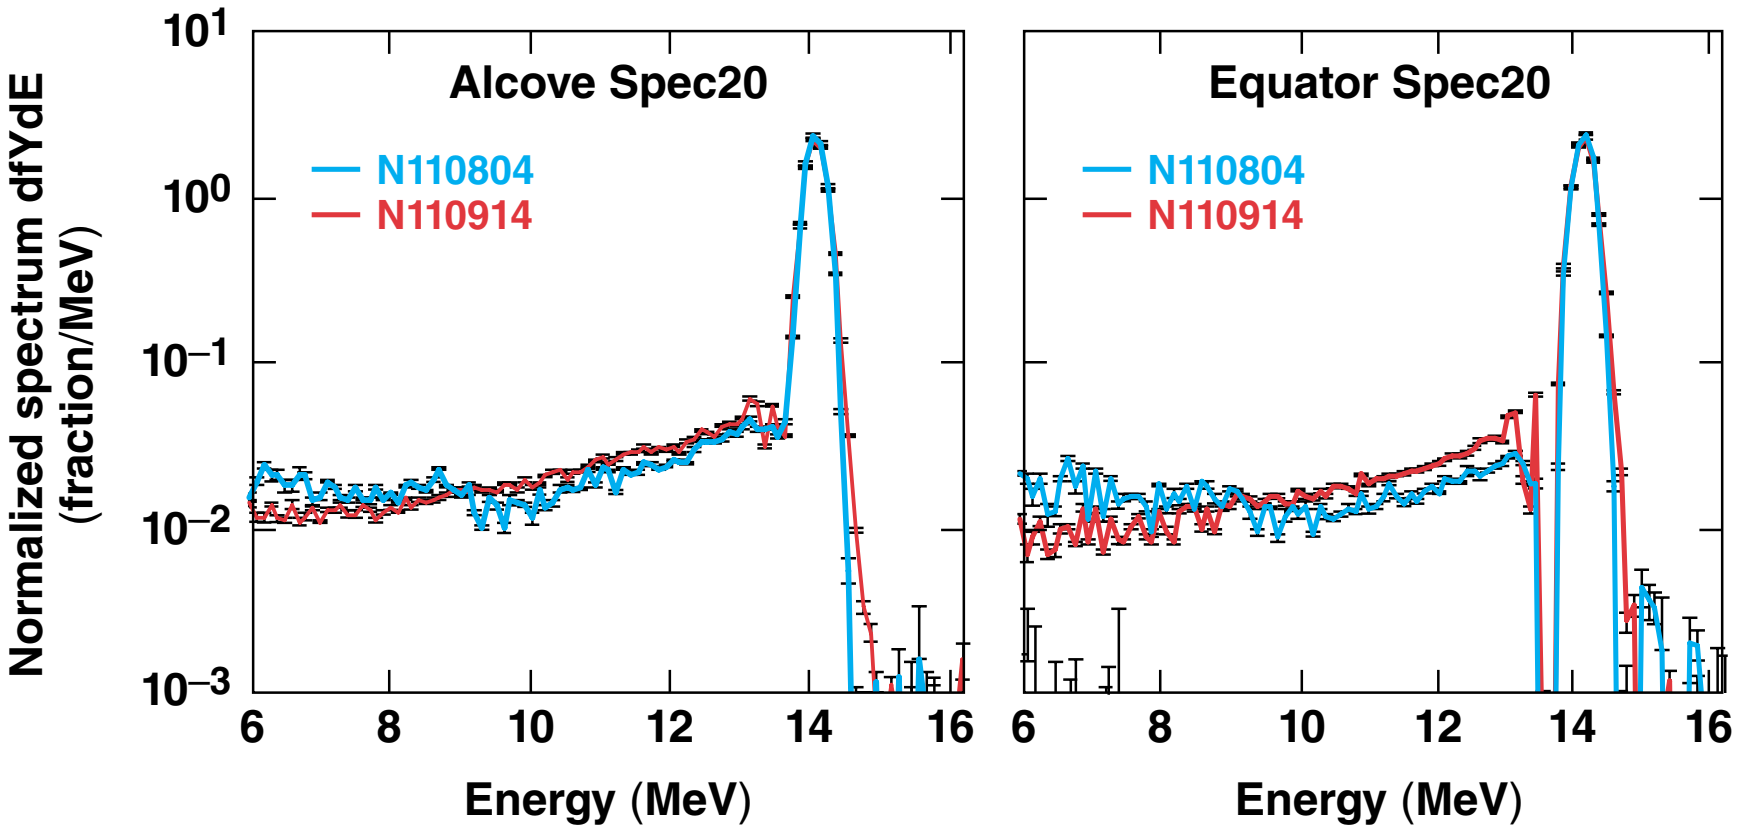

TT neutrons seen for energies <9.3 MeV

E20364

Summary/Conclusions

High-quality data from NIF Spec20 detectors make it possible for neutron spectra to be calculated from a deconvolution

- Instrument response function (IRF) determined from *in-situ* measurements
- Spec20 detectors probe NIF implosions from two different lines-of-sight
- Neutron spectra are calculated with an error analysis built into the deconvolution

Deconvolution of neutron spectra allow for a generalized DSR to be calculated.

Convolution of DT peak with IRF does not match layer shot data

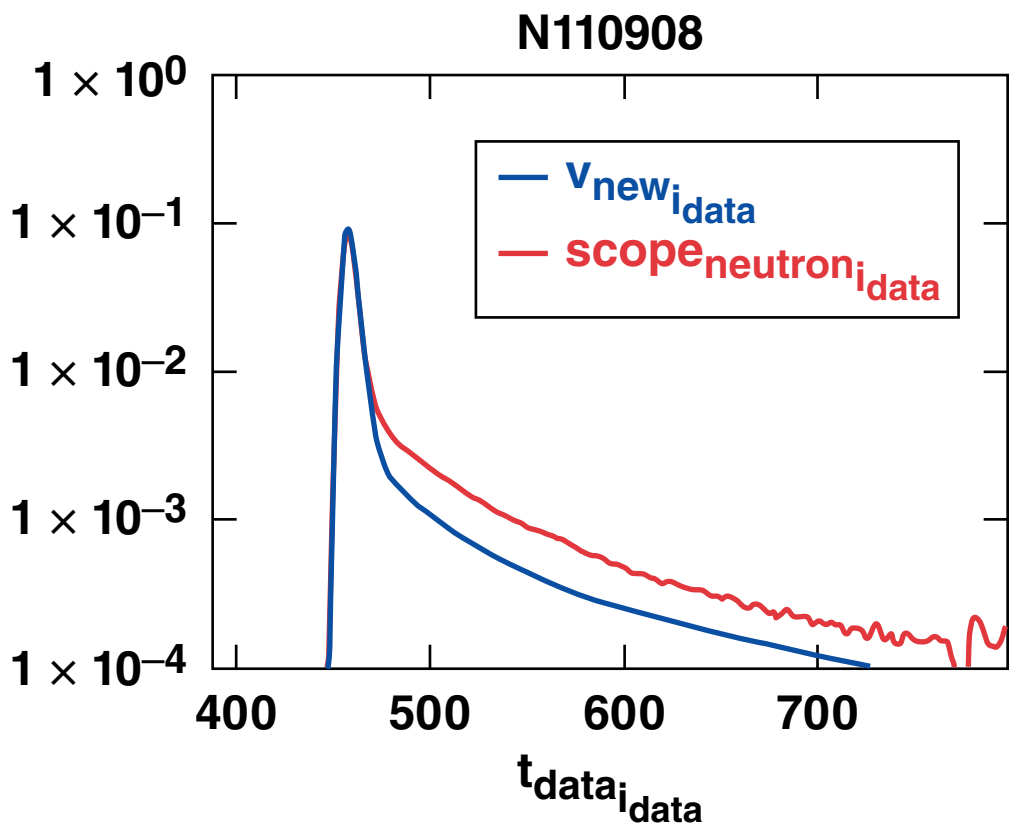

E20365

Convolution of DT peak with IRF matches data from 1.6-mm exploding-pusher shell

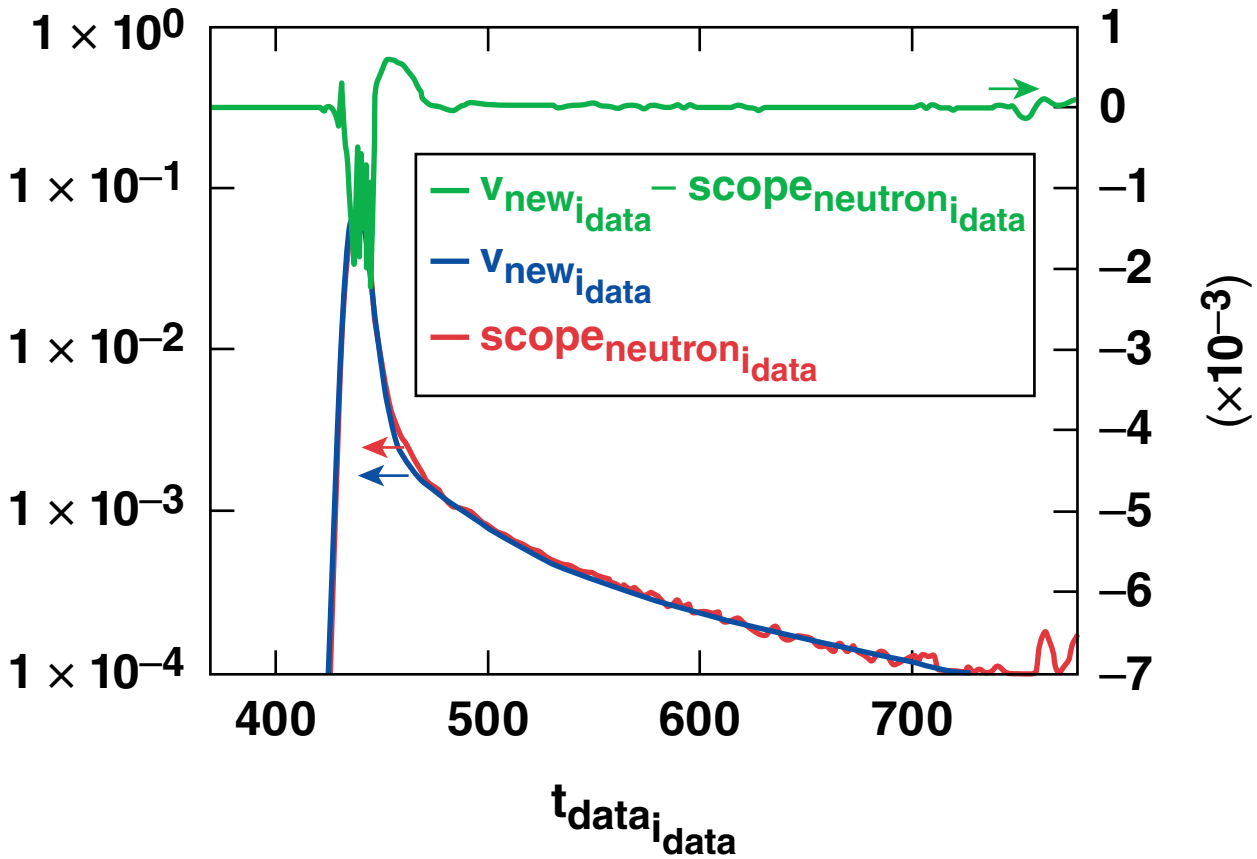

Forward convolution of deconvolved model agrees with measured data.

E20366

Deconvolution of IRF enhances the signal to background in the DSR region

- Layered shot data shown as red line
- Exploding-pusher shot data shown as points; time > 14.9-ns data multiplied by 20 to show signal background
- DSR $\equiv Y_{10\text{ to }12}/Y_{13\text{ to }15}$

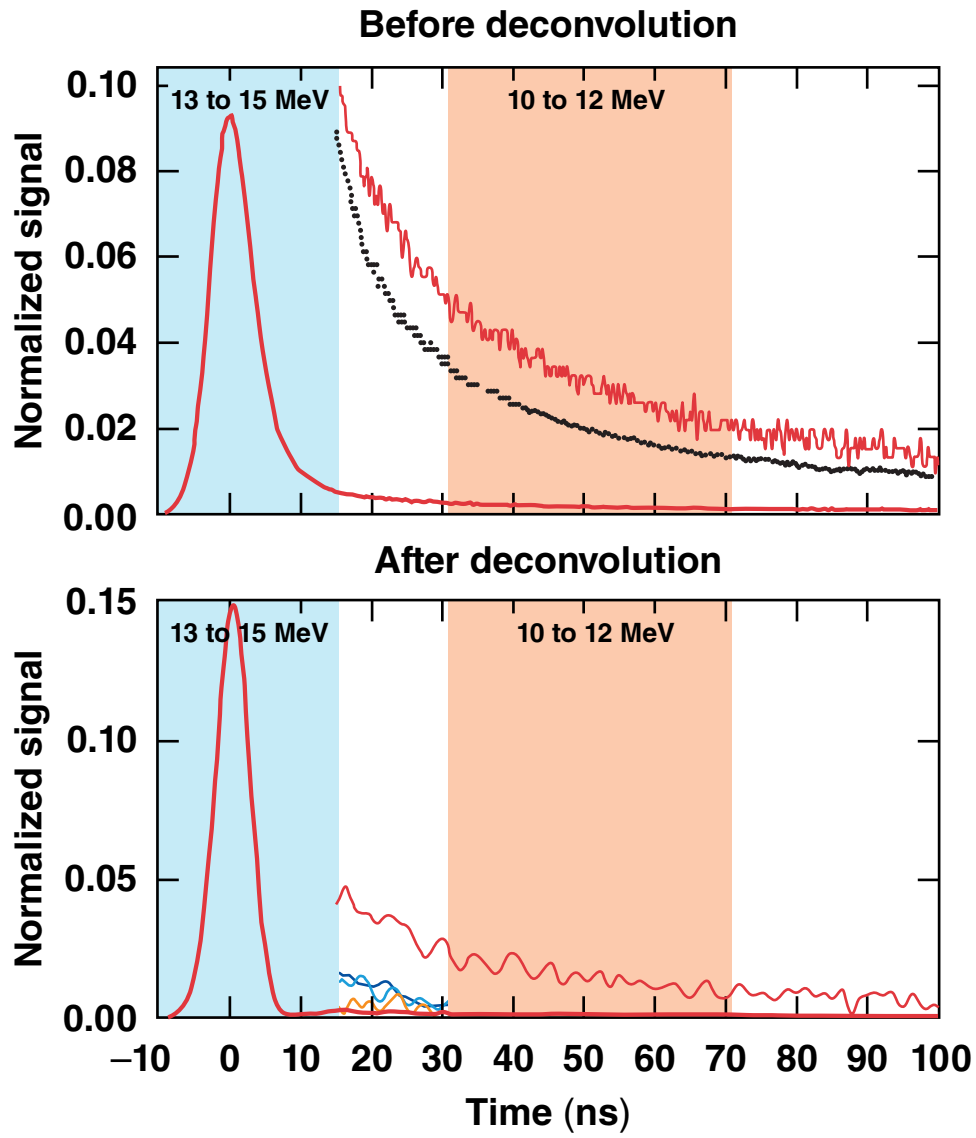

E20100a

Two nTOF Spec20 detectors are installed on the NIF target chamber

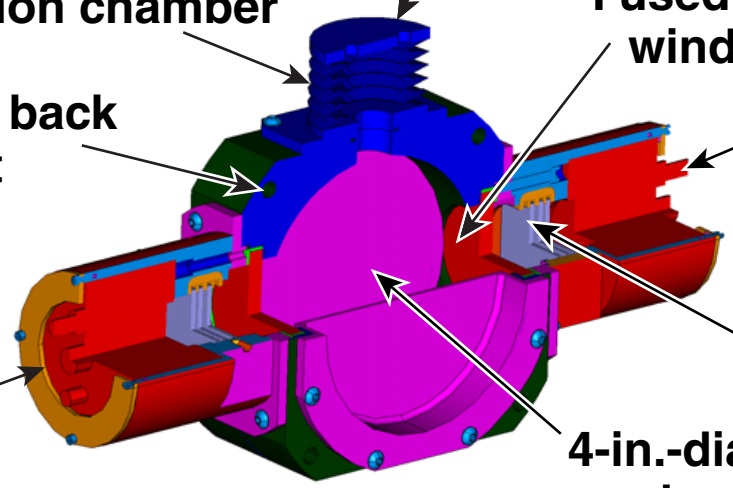

Equator installation 20 m from tcc
Alcove installation 22 m from tcc

nTOF Spec20 has been calibrated with DT and D_2 implosions on both OMEGA and the NIF.

E20368